



Data logger for various on-site measurements


PORTABLE DATA LOGGER TS-360



Tokyo Measuring Instruments Laboratory Co., Ltd.

T-ZFICES 3 PORTABLE TS-360

Features



- LAN communication with remote measurement assistance function
- Low power consumption operation
- Measurement speed 0.08 sec/point*0.2 sec/point when measured by TML-NET
- External switch box can connect up to 20 units,1000 points, 2 km when booster power is turned on
- Channel unit AU-10/AU-10-05:

 Color LED lights up when measuring

 (Strain [red]/DC voltage [blue]/Thermocouple [green])

Point

Up to 1000 points

Number of measurement points up to 50 points connected to the main unit

External connection: up to 1000 points total

2. LAN interface as standard

Remote control is available!

3. TML-NET Compatible

100 units can be connected with TML-NET

5. Battery-powered operation

Powered by 4 single batteries or AC adapter (12V battery).

4.


Connection to Switching box

T-ZACCS BOX AU-50, ASW-50C, and SSW-50D can be connected as an external switching box!

Application

For example, you can do this!





Pavement



TS-360 is battery-operated, making it powerful in places where there is no power supply!



Connecting to an external switch box, up to 1000 points can be used, making it useful for multi-point field measurements!



Slope and mountain area



"TML-NET" can be used. Therefore, it can be used at landslide and water level observation sites where measurement points are scattered



Supports sleep interval measurement, ideal for unattended measurement using dry cell batteries or batteries at sites that are distant or difficult to access!




Bridge



When used in connection with an external switch box, you can have the right number of points where you need them!



TS-360 also supports online measurement by connecting I/F (LAN, USB, RS-232C)!



Tunnel




TS-360 can increase the number of points and distribute placement as construction progresses!



T-ZACCS BOX AU-50 can be connected as an external switch box. Existing switch box ASW-50C/SSW-50D can also be connected!


T-ZFICES 3 PORTABLE TS-360

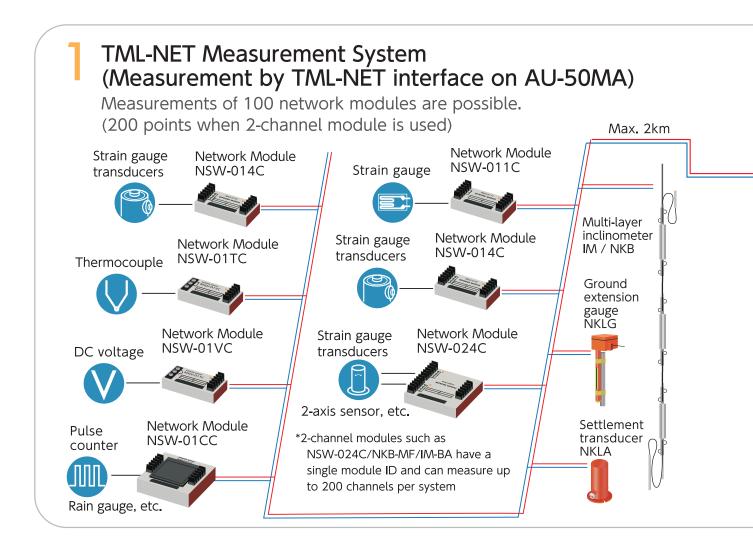

External Switching box measurement system

T-ZACCS BOX AU-50 and conventional switching boxes ASW-50C /SSW-50D can be used (can be mixed)!

Capable of measuring up to 1000 points.

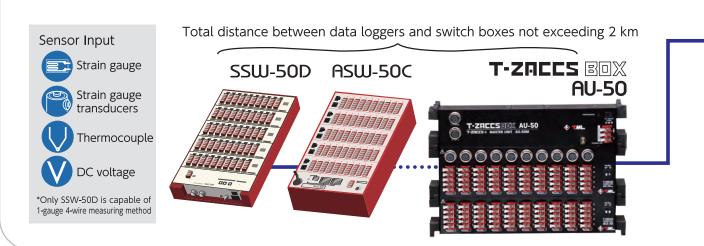


System Block Diagram



Software

External Printer



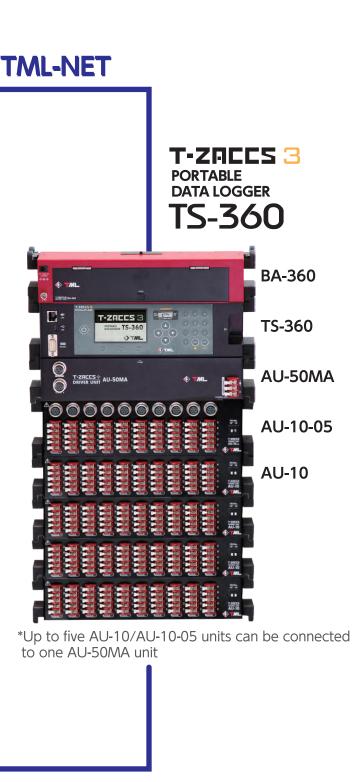

External Switching box

T-ZACCS 3 PORTABLE DATA LOGGER TS-360

T-ZACCS 3

Control unit TS-360



Measuring capacity

Number of mea	Number of measurement points Up to 1000 points					
Measuring	Scanning	0.080 sec/point (50Hz)				
speed	measurement	0.067 sec/point (60Hz)				
speed	Monitor measurement	0.5 sec/point				
Measureme	nt mode	Initial, Direct, Major				
Measurenie	iit iiiode	(Temperature measurement is direct only)				
		Coefficient 1				
Simple Meas	sure	Unit Linked to sensor mode				
		Decimal point Linked to sensor mode				
Comet settii		Comet NON, Comet A, Comet B				
		OFF, numerical value, scan				
Monitor	Display	numeric representation 1 to 8 points				
	channel	Scanning display 1 to 1000 points				
	Manual Measurement					
measurement		Interval measurement, Comparator measurement				
	interface	LAN, USB, RS-232C				
	Coefficient	± (0.00000~200000)				
	Unit	με, mV, ℃, kgf, mm etc.,				
	Decimal point	Decimal point display can be set to 0 to 5 optional digits				
	Offset	Writing for each arbitrary measurement channel				
		Set the type of sensor to be connected				
Channel setting		Quarter bridge 3-wire 120/240/350Ω				
		Strain Quarter bridge 4-wire120/240/350Ω				
	Sensor mode	measurement Half bridge common dummy, Half bridge				
		Full bridge, Full bridge constant current350Ω				
		Voltage 300mV, 30V				
	D. 1	Temperature Thermocouple T, K, J, B, S, R, E, N				
	During measurement	Open check				
Charle from atten	C	Insulation check, sensitivity check, variation check, thermocouple disconnection check, lead wire resistance				
Check function	Sensor	check, bridge output check, coefficient check				
	Disalau astina list	<u> </u>				
	Display setting list	Initial value, lead wire resistance				

^{*}Quarter bridge 4-wire is available only for SSW-50D. (As of February 2024)

Interval measurement

inter tal medeal emerit				
Function	Recording of measurement values at set time interval and time			
Time interval	Hours, minutes, seconds, up to 99 hours 59 minutes 59 seconds Can be set for each step			
Real time start	Start time (hour, minute, seconds) can be set for each step			
Number of start	Up to 9999 times per step or infinite			
Number of steps	Programmable up to 10 steps			
GOTO step	Program loop possible to one of the previous steps			
GOTO comparator	Go to step 1 of the comparator			
Sleep function	Automatically turns power on and off at intervals of 1 minute or more between the end of a scan and the start of the next scan			

Comparator measurement

Function	Automatic measurement by the amount of change in the setting of any channel (one point)
Comparative amount	Up to ±999999 settable per step
Comparison method	Upper/lower limits, relative values
Number of start	Up to 9999 times per step or infinite
Number of steps	Programmable up to 10 steps
GOTO step	Program loop possible to one of the previous steps
GOTO interval	Go to step 1 of the interval

Time

Setting	Year, month, day, hour, minute, seconds
Accuracy	Daily error: ± 1 seconds (@23℃ ± 5℃)
Retention	Approx. 30 days (with full charge)

Display and Operation

Display		LCD panel	3.0 semi-transmissive monochrome STN LED backlight
	Display unit	Resolution	3.0 semi-transmissive monochrome STN LED backlight 255×160 dots 10 dots or less (excluding aging deterioration)
		Point defect	10 dots or less (excluding aging deterioration)
Operation			POWER, START, ESC, ENT, 0 to 9, F1, F2, F3

Recording

D	Dutle to	Function	Recording and reproduction of measurement data Saving of setting file			
В	uilt-in	Recording format	CSV format, TDS format			
		Capacity	16 GB			
	SD card	Function	Recording, reproduction, copying of measurement data Saving of setting file			
SI		Physical format	FAT32			
		Recording format	CSV format, TDS format			
		Capacity	16 GB (Designated by us)			

Interface

LAN	10BASE-T/100BASE-TX General-purpose command port server function (various settings, measurement, data collection)
USB	USB 2.0 protocol compatible Various settings, measurements, data collection
RS-232C	RS-232C compliant Baud rate 9600, 38400, 115200 bps Various settings, measurements, data collection

Power supply

Power supply voltage	DC9~18V50/60Hz

Environment

	(Operating temperature/humidity range		-10∼+50℃	85%RH	or	less	(No	con	dens	ation	١)
--	---	--------------------------------------	--	----------	-------	----	------	-----	-----	------	-------	----

Others

External dimensions	280(W)×45(H)×80(D)mm (Excluding rubber protectors and protrusions)
weight	Approx. 800g

Standard accessories

instruction manual for standard accessories(CD)	1
SD card	1
Phillips screwdriver	1
Warranty card	1 copy

Options

SD card	16 GB (Designated by us)		
AC adapter	CR-1867		
RS-232C Cable	CR-5360		
USB cable	Type C USB Cable		
External Printer	DPU-S245 (RS-232C connection)		

Specification 仕様

T-ZACCS+

Driver unit AU-50MA



Measurement capability

Number of measurement points	When using box connection When using box connection and built-in measurement unit together Channel unit connection		
Data update cycle		0.080 sec/point (50h 0.067 sec/point (60h	Hz) Hz)
Measurem	ent Mode	Direct	
Applicable wiring methods.	Quarter bridge 3-wire Half bridge Half bridge common dummy	120/240/350Ω 120~1000Ω 120~1000Ω	
	gauge resistance	Full bridge Full bridge constant current	120~1000Ω
Strain measurement	Sensor cable extension range	Full bridge constant current 350Ω	Total cable resistance: 400 Ω or les
	Sensitivity change	ŭ .	for total cable resistance 100 Ω
	Lead wire resistance	Gauge resistance 120Ω	
	compensation range	Gauge resistance 240Ω	
	CometB(1G3W)		: About 300Ω or less
	Zero stability	±1.0×10-6 strain/°C or less (quarter bridge) ±0.5×10-6 strain/°C or less (half bridge)	
	Initial unbalance	±500×10-° strain or less (half bridge)	
DC voltage	Input impedance	1MΩ or more	
measurement Allowable input voltage between B and D			
Thermocouple temperature measurements		T, K, J, B, S, R, E, N JIS C1602:2015 IEC6	0584-1:2013
Check function	During measurement	Open check	
	sensor	Insulation check, sensitivity check, disconnection check, lead wire resi	variation check, thermocouple istance check, bridge output check

Strain measurement

ou diri mododi omore		
Bridge power supply	DC2V 24ms(50Hz)	
Initial value storage range	±160000×10-6strain	
Temperature coefficient of accuracy	±0.002% rdg/C	
Aging change of accuracy	±0.02% rdg/year	
	Measuring range	Resolution
Measuring range and resolution	± 30000×10 ⁻⁶ strain	1×10 ⁻⁶ strain
	±300000×10-6 strain	10×10-6 strain
Accuracy (@23°C±5°C)	 ±(0.08%rdg+1digit)	
(Except quarter bridge 4-wire)	= (0.00% ag 1 Taigit)	
Accuracy (@23℃±5℃)	±(0.28%rdg+1digit)	
Quarter bridge 4-wire	-(0.20/014g 1 Talgit)	

Constant current strain measurement(Full bridge)

Bridge Power Supply	DC6mA 24ms(50Hz)	
Bridge resistance	350Ω	
Initial value storage range	±160000×10-6 strain	
Temperature coefficient of accuracy	±0.002%rdg/°C	
Aging change of accuracy	±0.02%rdg/year	
	Measuring range	Resolution
Measuring range and resolution	± 30000×10 ⁻⁶ strain	1×10 ⁻⁶ strain
	±300000×10-6 strain	10×10-6 strain
Accuracy(@23℃±5℃)	±(0.08%rdg+3digit)	

DC voltage measurement

Initial value storage range			
V1/1		±160.000mV	
V1/100		±16.0000V	
Temperature coefficient of accuracy		±0.0024%rdg/℃	
Aging change of accuracy		±0.024%rdg/year	
	V1/1	Measuring range	Resolution
		± 30.000mV	0.001mV
Measuring range and resolution		±300.000mV	0.010mV
	V1/100	± 3.0000V	0.0001V
		±30 . 0000V	0.0010V
Accuracy (@23℃±5℃)	V1/1	±(0.08%rdg+3digit)	
	V1/100	±(0.08%rdg+2digit)	

Thermocouple measurement accuracy

	Accuracy (@22°+E°)			(@22°C + E°C)
Type	Measuring range	Resolution	,	(@23℃±5℃)
. /			External reference junction	Internal reference junction
	−250~−200°C	0.1°C	±(0.38%rdg+0.6°C	±(0.38%rdg+3.9°C)
T	-200~-100°C	0.1°C	±(0.15%rdg+0.2°C)	±(0.15%rdg+1.4°C)
	-100~+400°C	0.1°C	±(0.10%rdg+0.2°C)	±(0.10%rdg+0.8°C)
	-210~-160°C	0.1°C	±(0.19%rdg+0.3°C)	±(0.19%rdg+1.6°C)
K	-160~0°C	0.1°C	±(0.12%rdg+0.2°C)	±(0.12%rdg+1.0°C)
	0~+960°C	0.1°C	±(0.08%rdg+0.1°C)	\pm (0.08%rdg+0.5°C)
	+960~+1370°C	0.1°C	±(0.10%rdg+0.9°C)	±(0.10%rdg+1.4°C)
	-200~-160°C	0.1°C	±(0.16%rdg+0.2°C)	±(0.16%rdg+1.2°C)
1 .	-160~0°C	0.1°C	±(0.12%rdg+0.1°C)	±(0.12%rdg+0.8°C)
J	0~+700°C	0.1°C	±(0.08%rdg+0.1°C)	±(0.08%rdg+0.5°C)
	+700~+1200°C	0.1°C	±(0.08%rdg+0.6°C)	±(0.08%rdg+0.9°C)
	+200~+280°C	0.5~0.4°C	±(0.04%rdg+4.0°C)	±(0.04%rdg+4.0°C)
В	+280~+800°C	0.3~0.1°C	±(0.04%rdg+1.2°C)	±(0.04%rdg+1.2°C)
	+800~+1760°C	0.1°C	±(0.05%rdg+0.4°C)	±(0.05%rdg+0.4°C)
S	-10~+200°C	0.1°C	±(0.09%rdg+0.6°C)	±(0.09%rdg+1.2°C)
)	+200~+1760°C	0.1°C	±(0.07%rdg+0.4°C)	±(0.07%rdg+0.7°C)
	-10~+150°C	0.1°C	±(0.09%rdg+0.7°C)	±(0.09%rdg+1.2°C)
R	+150~+1760°C	0.1°C	±(0.07%rdg+0.4°C)	±(0.07%rdg+0.7°C)
	-210~+550°C	0.1°C	±(0.17%rdg+0.2°C)	±(0.17%rdg+1.4°C)
E	+550~+1000°C	0.1°C	±(0.09%rdg+0.4°C)	±(0.09%rdg+0.8°C)
	-200~0°C	0.1°C	±(0.18%rdg+0.4°C)	±(0.18%rdg+1.6°C)
N	0~+1090°C	0.1°C	±(0.08%rdg+0.2°C)	±(0.08%rdg+0.6°C)
	+1090~+1300°C	0.1°C	±(0.08%rdg+0.9°C)	±(0.08%rdg+1.2°C)

^{*}The accuracy of sensor is not included, and thermocouple B does not use a reference junction

Switching box drive unit

Compatible model		SSW-50D, ASW-50C
		AU-50M
No. of units	Without booster power	8 units connected, 400 points
	Booster power available	20 units connected, 1000 points
distance	Without booster power	120m
	Booster power available	2km
Connection cable		Switch box cable (CR-65) or switching box extension cable (CR-800)

Compatible model		NSW series/TML-NET compatible transducers
		Up to 100 units
		Up to 20 units (150m or less)
Extension	Low consumption type	2km
distance	Existing type	Within 1 km (10 units or less)
Connection cable		Dedicated 2-conductor shielded cable

Channel unit connection

Compatible model	AU-10/AU-10-05
No. of units connected	Up to 5 units
Connectors	Dedicated connector for unit connection

Power

Supply power	Supplied by TS-360

Environment

Other

	280 (W)×45 (H)×60 (D) mm (Excluding rubber protectors and protrusions)
Weight	Approx. 800g

Standard accessories

Warranty card	1 copy
---------------	--------

T-Z月CCS 3 Specification 仕様

T-ZACCS UNIT

Channel unit AU-10/AU-10-05



Function

Number of measuring point	10
	Dual-use screw and solder type
One-touch connector	NDIS One-touch connector(AU-10-05 only)
Measuring capacity	Equivalent to AU-50MA/AU-50M

Power

Supply power	Supplied by AU-50MA/AU-50M
--------------	----------------------------

Environment

Operating temperature/humidity range -10~+50℃ 85% RH or less (excluding condensation)

Other

External dimensions	AU-10 280 (W) × 45 (H) × 60 (D) mm AU-10-05 280 (W) × 45 (H) × 80 (D) mm (Excluding rubber protector and projection)
Weight	AU-10 Approx, 900g AU-10-05 Approx, 1,2kg

Standard accessories

Warranty card	1 copy
---------------	--------

T-ZACCS+

Battery unit BA-360



Function

Function	Ability to run TS-360 on a single battery
Batteries	4 single alkaline dry cells
Usable time	Continuous usage : Approx. 40 hours At 1-hour interval : Approx. 8 months (10 channels, scan, sleep on, 23±5°C)

Environment

Operating temperature/humidity range -10~+50°C 85% RH or less (excluding condensation)

Other

		280(W)×60(H)×60(D)mm
	(Excluding rubber protector and projection)	
	Weight	Approx. 1.2 kg (including 4 single dry cells)

Standard accessories

Single alkaline dry cell	4
Warranty card	1 copy

Expandable by unit! T-ZRCCS BOX AU-50

The AU-50 consists of a master unit and a channel unit.

It can be used with TS-360, TDS-540, etc. and can be mixed with conventional switchboxes ASW-50C/SSW-50D.

1 to 5 channel units can be added to the Master unit

T-ZACCS+

Master unit **AU-50M**



Channel unit AU-10/AU-10-05







Approval Certificate ISO9001 Design and manufacture of strain gauges, strain measuring equipment and transducers The contents of this catalog are subject to change without prior notice. The contents of this catalog are as of July 2024. TML Pam E3021C.



8-2, Minami-ohi 6-chome, Shinagawa-ku, Tokyo 140-8560, JAPAN TEL: +81-3-3763-5614 FAX: +81-3-3763-6128

